

2000

# Flow injection solid phase extraction with Chromosorb 102: determination of lead in soil and waters by flame atomic absorption spectrometry

L Elci

Z Arslan

JF Tyson

Follow this and additional works at: [https://scholarworks.umass.edu/chem\\_faculty\\_pubs](https://scholarworks.umass.edu/chem_faculty_pubs)

 Part of the [Chemistry Commons](#)

---

## Recommended Citation

Elci, L; Arslan, Z; and Tyson, JF, "Flow injection solid phase extraction with Chromosorb 102: determination of lead in soil and waters by flame atomic absorption spectrometry" (2000). *Spectrochimica Acta Part B-Atomic Spectroscopy*. 1044.  
Retrieved from [https://scholarworks.umass.edu/chem\\_faculty\\_pubs/1044](https://scholarworks.umass.edu/chem_faculty_pubs/1044)

This Article is brought to you for free and open access by the Chemistry at ScholarWorks@UMass Amherst. It has been accepted for inclusion in Chemistry Department Faculty Publication Series by an authorized administrator of ScholarWorks@UMass Amherst. For more information, please contact [scholarworks@library.umass.edu](mailto:scholarworks@library.umass.edu).

# Flow injection solid phase extraction with Chromosorb 102: determination of lead in soil and waters by flame atomic absorption spectrometry <sup>☆</sup>

Latif Elçi<sup>a,\*</sup>, Zikri Arslan<sup>b</sup>, Julian F. Tyson<sup>b</sup>

<sup>a</sup>Department of Chemistry, Erciyes University, Kayseri, TR-38039, Turkey

<sup>b</sup>Department of Chemistry, University of Massachusetts, Amherst, MA 01003-4510, USA

Received 22 September 1999; accepted 24 February 2000

---

## Abstract

A flow-injection, solid-phase extraction, preconcentration method was developed for the determination of lead in soil and water samples by flame atomic absorption spectrometry. Lead, in the form of the diethyldithiocarbamate complex, was retained on a miniature column of Chromosorb 102 from buffered sample solutions. Several parameters governing the efficiency and throughput of the method were evaluated including pH, eluent composition, volume and flow rate. The complex retained from pH 9.0 (ammonium acetate) solutions was eluted with 1.76 µl of ethanol, at 4.2 ml min<sup>-1</sup> into the nebulizer–burner system of the spectrometer. The detection limit was 2 µg l<sup>-1</sup> for preconcentration at 2.2 ml min<sup>-1</sup> for 120 s. The relative standard deviation (R.S.D.) was less than 4% for concentrations down to 400 µg l<sup>-1</sup>. The procedure was validated by the analysis of NIST standard reference material 2711 (Montana Soil) which contains lead at a concentration of 1162 µg g<sup>-1</sup>. Recoveries of spike additions (100–400 µg l<sup>-1</sup>) to artificial sea water and tap water were quantitative.

**Keywords:** Flow injection; Solid phase extraction; Pb; Soil; Flame atomic absorption spectrometry

---

## 1. Introduction

There is an on-going need to determine lead because of its extensive distribution and high

toxicity. Flame atomic absorption spectrometry (FAAS) is, in principle, a suitable technique as it is rapid, simple and inexpensive; however, lead concentrations in matrices such as biological materials, soil, natural water, environmental, and food samples are such that, typically, the concentrations in sample extracts or digests are below the detection limit of FAAS. In addition, high concentrations of matrix components (including the acids used for sample dissolution or digestion) may cause inaccuracies in a method which is

---

<sup>☆</sup> This paper was presented at Colloquium Spectroscopicum Internationale XXXI, held in Ankara, Turkey, September 1999, and is published in the Special Issue of *Spectrochimica Acta Part B*, dedicated to that conference.

\* Corresponding author. Fax: +90-352-437-0782.

E-mail address: elci@erciyes.edu.tr (L. Elçi).

based on external calibration with dilute aqueous standards. Therefore, a preconcentration and/or separation is needed to improve the detection limit and selectivity for the determination of lead by FAAS. Flow injection (FI) techniques for preconcentration and separation coupled with FAAS have been used for this purpose [1,2], and several solid phase extraction (SPE) procedures have been developed for the determination of lead [3–12]. The most extensively used extractant is C-18 silica [8–12], though various other materials, including activated carbon [13], alumina [14], cellulose [15], and Amberlite XAD-8 have been used [16].

It would appear that the most successful general approach is to use a hydrophobic solid phase extractant for the retention of a non-polar derivative of the target analyte. A class of hydrophobic materials that, to our knowledge, has not been investigated for use in FI-SPE procedures is the various non-polar gas chromatography (GC) stationary phases. Chromosorb 102, (a styrene-divinyl-benzene copolymer) has been extensively used in gas chromatography for the separation of organic compounds such as hydrocarbons, alcohols, pesticides and aromatics in a variety of samples [17–19].

To demonstrate the feasibility of this material as a solid phase extractant for use in FI-AAS, we have used it in a procedure for the determination of lead by retention from alkaline solution as the diethyldithiocarbamate complex, followed by elution with a discrete volume of ethanol. The procedure was applied to the analysis of tap water, artificial sea water, and a certified reference soil. In the development of the procedure, a number of parameters relevant to the retention and elution of the analyte were investigated, but no attempt was made to develop a fully automated procedure.

## 2. Experimental

### 2.1. Apparatus

A Perkin-Elmer (Norwalk, CT, USA) Model 1100 B atomic absorption spectrometer with deuterium background correction, equipped with a

10-cm air-acetylene burner, was used. An intensitron (Perkin-Elmer) lead hollow cathode lamp, operated at 7 mA, was used at 283.3 nm with a 0.7-nm spectral bandpass. Data were recorded by an Epson Model LQ-850 printer. An air-acetylene flame was employed with gas flow rates of 6.0 and 2.5 l min<sup>-1</sup> for air and acetylene, respectively. The nebulizer uptake rate and position of the capillary in the venturi throat were adjusted to obtain the maximum absorbance for conventional sample introduction (approx. 6.0 ml min<sup>-1</sup>).

A Perkin-Elmer FIAS-200 unit with a six-port rotary flow injection valve was used as the sample introduction system. The schematic diagram of the FI manifold for preconcentration and matrix

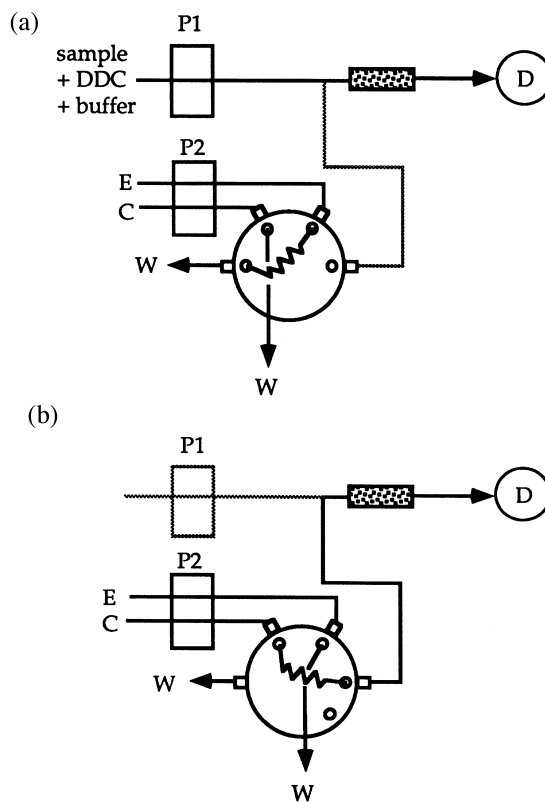


Fig. 1. Schematic diagram of the flow injection manifold: P<sub>1</sub>, sample pump; P<sub>2</sub>, eluent and carrier pump; D, detector; C, carrier; E, eluent; and W, waste. (a) Sample loading position; after pump 1 is turned off, pump 2 runs for 10 s to fill the injection loop. (b) Elute position; the valve is turned to deliver a discrete volume of the eluent.

separation is shown in Fig. 1, and the FIAS program is given in Table 1. Tygon pump tubes (1.52 mm i.d.) were used for sample, ethanol and carrier solutions. All connecting tubings were made of 0.8 mm i.d. PTFE.

For the microwave digestion of the soil samples a CEM (Indian Trail, NC, USA) Model MSD-81D oven, providing  $630 \pm 70$  W output power at the 100% power setting, was used. The 12-vessel turntable drive system rotates the samples  $360^\circ$  within the microwave field at  $6 \text{ rev. min}^{-1}$ . The vessel body and the cap are made of polyetherimide (Ultem), and the liner, cover and the rupture membrane are made of Teflon<sup>®</sup>-perfluoroalkoxy (PFA). The vent screw is constructed of PTFE. The volume of the liner is 100 ml.

## 2.2. Reagents and samples

All reagents used were of analytical reagent grade. High-purity deionized water ( $18 \text{ M}\Omega \text{ cm}$ ) was used throughout the experiments. Diethyldithiocarbamic acid diethyl ammonium salt (Aldrich) was used for daily preparation of 0.5% m/v  $\text{NH}_4\text{DDC}$  solution by dissolving 0.05 g of solid  $\text{NH}_4\text{DDC}$  in ammonium acetate buffer solution ( $0.06 \text{ M NH}_3 + 0.03 \text{ M CH}_3\text{COOH}$ , pH 9). The DDC solution was passed through a column

packed with Chromosorb 102 resin to eliminate possible contamination prior to the addition into standard and sample solutions. Standard solutions of lead were prepared daily in the concentration range of  $0.05\text{--}0.6 \mu\text{g ml}^{-1}$  by appropriate dilution of a  $1000\text{-mg l}^{-1}$  stock solution (Aldrich). Ethanol was used as the eluent.

Chromosorb 102 resin, a porous styrene-divinylbenzene copolymer, (Phase Separations Inc., Norwalk, CT, USA) having a surface area of  $300\text{--}400 \text{ m}^2 \text{ g}^{-1}$  and a particle size of  $80\text{--}100$  mesh was used as the solid phase extractant. This hydrophobic resin can be used in a pH range from 0 to 14 [20]. Artificial sea water (250 ml) was prepared by dissolving 0.3675 g of  $\text{CaCl}_2 \cdot 2\text{H}_2\text{O}$ , 3.275 g of  $\text{MgSO}_4 \cdot 7\text{H}_2\text{O}$  and 6.975 g of NaCl in deionized water [21]. The pH values of the test solutions were adjusted to pH 9.0 by dropwise addition of  $\text{NH}_3$  and  $\text{CH}_3\text{COOH}$  solutions before use.

## 2.3. Method development

The column, a glass tube of 45 mm long and 2.3 mm i.d., was dry-packed with 110 mg of Chromosorb 102 resin. A small amount of glass wool was placed at both ends of the column to prevent loss of the resin beads during sample loading. The

Table 1  
FIAS-200 program

| Step no. | Time (s) | Pump 1 (rev. $\text{min}^{-1}$ ) | Pump 2 (rev. $\text{min}^{-1}$ ) | Valve position | Remarks   |
|----------|----------|----------------------------------|----------------------------------|----------------|---|
| 1        | Variable | 50                               | Off                              | Fill           | Preconcentration — sample pumped through column for a maximum of 99 s                 |
| 2        | Variable | 50                               | Off                              | Fill           | Second stage needed for preconcentration time greater than 99 s                       |
| 3        | 10       | Off                              | 100                              | Fill           | Injection loop filled with ethanol, carrier flushes unretained components from column |
| 4        | 15       | Off                              | 100                              | Elute          | Valve switches to elute position, slug of ethanol flushed through column              |

resin bed was approximately 40 mm long. For the conditioning of the column, ammonium acetate buffer solution (pH 9.0) which contained 0.5% m/v DDC, was passed through the column which was then washed with ethanol and water several times. After each elution, the column was ready for re-use without further pretreatment. In addition, the performance of the column was evaluated daily by preconcentrating a  $0.4\text{-}\mu\text{g ml}^{-1}$  Pb solution for 60 s.

The effect of pH on the retention of lead was examined over a pH range of 4–10. Lead standard solutions containing  $0.4\text{ }\mu\text{g ml}^{-1}$  Pb were loaded onto the column after complexing with DDC. The flow rate of the sample solution ( $0.4\text{ }\mu\text{g ml}^{-1}$  lead) was varied from 1.3 to  $5.0\text{ ml min}^{-1}$  to investigate the effect on the retention of lead on the column. The volume of the eluent was varied over the range of 50–200  $\mu\text{l}$ , and the eluent flow rate, for 176  $\mu\text{l}$  of ethanol, was varied from 2.9 and  $5.0\text{ ml min}^{-1}$ . For the elution of the Pb-DDC complex from the column, ethanol, ethanol + 2% v/v HCl mixture (1 + 1), 1% v/v HCl, and 4%  $\text{HNO}_3$  were investigated. The flow rate of the carrier during these experiments was  $2.2\text{ ml min}^{-1}$ . The volume of 0.5% m/v DDC solution added to a 25-ml sample or standard solution was varied from 0 to 1000  $\mu\text{l}$ , while that of the buffer solution was varied from 0 to 25 ml.

For most studies, the figure of merit was maximum peak height; but, in the studies of the amount of reagents, the value of the blank signal was also taken into account.

#### 2.4. Method validation and procedures

A NIST soil reference material (SRM 2711, Montana Soil) was used for method validation. The soil was dissolved by a closed-vessel, microwave-assisted, digestion procedure [22]. Approximately 100 mg of the soil sample was digested in a mixture of 5.0 ml of sub-boiled  $\text{HNO}_3$  and 1.5 ml of HF at 240 W for 10 min [22]. At the end of the program, the vessels were removed and cooled to room temperature in a fume hood. After venting, the vessels were again tightly capped and irradiated for a further 10 min. This step was repeated twice. At the end of the third step,

complete dissolution was achieved yielding colorless solutions. The contents in the vessels were then diluted to 50 ml with water in a polyethylene calibrated flask. For the determination of Pb, either 1.0 or 2.0 ml of the original 50-ml solution was first neutralized by dropwise addition of the required volume of ammonia solution, and then diluted to 50 ml following the addition of 10.0 ml of the buffer solution (pH 9) and 100  $\mu\text{l}$  of 0.5% m/v DDC solution.

For recovery studies performed with artificial sea water, 8 ml of the buffer solution (pH 9) was first added to 40 ml of the sea water which was then spiked with either 5, 10 or 20  $\mu\text{l}$  of Pb ( $1000\text{ }\mu\text{g ml}^{-1}$ ). The solution was diluted to 50 ml with the buffer solution after adding 100  $\mu\text{l}$  of 0.5% m/v DDC solution. The concentration of Pb in the analysis solutions was either 0.1, 0.2 or  $0.4\text{ }\mu\text{g ml}^{-1}$ . Recovery studies were also performed with laboratory tap water. No further acid pretreatment was made for the tap water samples. All pH adjustments and additions were made as for the artificial sea water samples.

Sample and standard solutions were loaded onto the column with the FI manifold shown in Fig. 1. In the preconcentration step, the sample solution containing the lead-DDC complex in the buffer solution was pumped by Pump 1 at  $2.2\text{ ml min}^{-1}$ . The effluent was directly introduced to the nebulizer of the spectrometer. During the last 10 s of the preconcentration step (Step 3), Pump 2 was turned on and the loop of the valve filled with ethanol while the carrier (water) was directed to waste. The flow rate for both ethanol and water was  $4.2\text{ ml min}^{-1}$ . In the elution step, the valve was switched to the elute position, and the ethanol in the loop was flushed through the column by the water carrier. The Pb-DDC complex was eluted and introduced to the spectrometer. During elution, the carrier stream conditioned the column for the next preconcentration.

External calibration was performed with Pb standard solutions in the concentration range of 0, 0.05, 0.1, 0.2, 0.4 and  $0.6\text{ }\mu\text{g ml}^{-1}$ . Peak height absorbance was measured and five replicate measurements were made for each standard and sample solution. The calibration data were then processed on a personal computer using Excel

(Version 5.0) spreadsheet to obtain the calibration curve and the equation of calibration. The mean peak height absorbance for each sample solution was then substituted into the calibration equation to calculate the concentration of lead. Peak height was used as it was found that, for the sharp peaks typically obtained, the signal-to-noise ratio was better than that of peak area measurements. With the data handling capability available it was not possible to employ gated integration, and thus the integration window for peak area was sub-optimal.

### 3. Results and discussion

#### 3.1. Effect of chemical variables on preconcentration

The effect of the pH on the retention of Pb-DDC complex is shown in Fig. 2 for a  $0.4\text{-}\mu\text{g ml}^{-1}$  Pb standard solution. The maximum signal was obtained in basic solutions, in the pH range from 8 to 10. Thus, the pH was adjusted to 9 for subsequent experiments. For the various eluents, the highest signal was achieved with ethanol. Lower signals and incomplete elution (as evidenced by significant peaks for replicate elutions) of the Pb-DDC complex was observed for all the other solutions including ethanol + 2% HCl mixture (1 + 1), 1% v/v HCl, and 4% v/v  $\text{HNO}_3$ , which resulted in lower relative signals (approximately 45–60%). The volume of ethanol which gave the highest signal was 176  $\mu\text{l}$ . For lower volumes, relative signals were lower, probably due to incomplete elution. For volumes greater than 176  $\mu\text{l}$ , the signal decreased gradually because of the subsequent dilution of the analyte. No memory effects were observed for elution with 176  $\mu\text{l}$  of ethanol. The column was ready for the next sample after passing deionized water for 10 s following the appearance of the Pb signal.

The effect of sample flow rate ( $0.4\text{ }\mu\text{g ml}^{-1}$  Pb) is shown in Fig. 3. It can be seen that retention of the Pb-DDC complex was independent of flow rate from 1.3 to 2.2  $\text{ml min}^{-1}$ . Flow rates greater than 2.2  $\text{ml min}^{-1}$  resulted in lower signals which were interpreted as incomplete retention of the

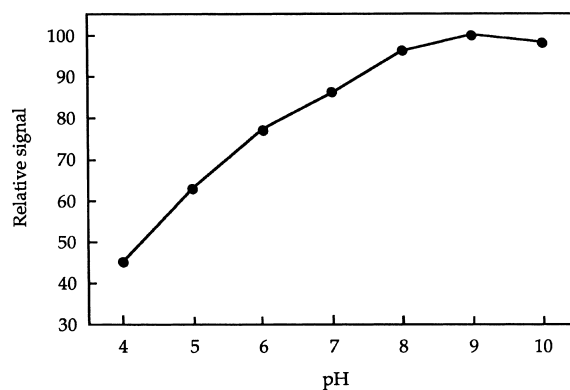


Fig. 2. Effect of pH on retention of Pb-DDC complex ( $0.4\text{ }\mu\text{g ml}^{-1}$  Pb solution).

Pb-DDC. Thus, the flow rate was kept at 2.2  $\text{ml min}^{-1}$  during the experiments. The effect of the eluent (ethanol) flow rate on the signal is also shown in Fig. 3. Maximum signal was achieved for flow rates between 3.8 and 5.0  $\text{ml min}^{-1}$ . For lower flow rates, the Pb signals were always lower. This was attributed to reduced nebulizer efficiency and dispersion of ethanol into the carrier stream, which could have resulted in the incomplete dissolution of the Pb-DDC complex. A carrier flow rate of 4.2  $\text{ml min}^{-1}$  was used.

The results for the effect of the concentration of 0.5% m/v DDC solution added into the 25-ml sample solution ( $0.4\text{ }\mu\text{g ml}^{-1}$  Pb) are given in Table 2. The minimum volume needed to achieve the maximum signal was 50  $\mu\text{l}$ , which yielded a

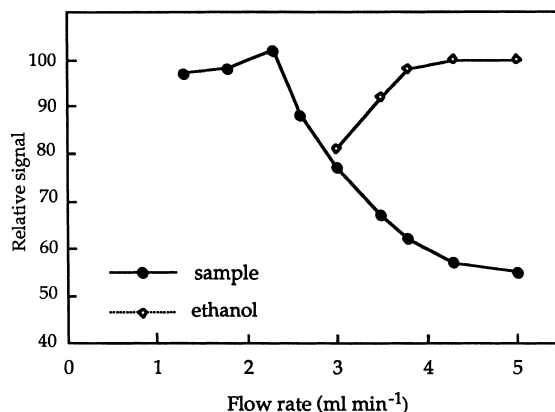


Fig. 3. Effect of sample and eluent flow rates.

Table 2

Effect of amount of DDC and buffer solutions on relative signal (25 ml sample volume solution;  $0.4 \mu\text{g ml}^{-1}$  Pb)

| 0.5% m/v DDC solution    |                     | Buffer solution (pH 9.0) |                     |
|--------------------------|---------------------|--------------------------|---------------------|
| Volume ( $\mu\text{l}$ ) | Relative signal (%) | Volume (ml)              | Relative signal (%) |
| 0                        | 56                  | 0.0                      | 55                  |
| 50                       | 100                 | 1.0                      | 67                  |
| 100                      | 100                 | 2.5                      | 76                  |
| 200                      | 95                  | 5.0                      | 99                  |
| 500                      | 100                 | 10.0                     | 100                 |
| 1000                     | 98                  | 15.0                     | 95                  |
|                          |                     | 25.0                     | 100                 |

DDC concentration of 0.001% m/v in the 25-ml solution. No significant differences were observed in the Pb signals when the volume of DDC solution was increased up to 1.0 ml. Although Pb was retained on the column even in the absence of DDC, the relative signals were low (approx. 56%). This phenomenon was not investigated in further in this study; however, it has been examined as the basis of a possible multi-element preconcentration procedure [23]. The minimum volume of the ammonium acetate buffer solution to adjust the pH of the solution to 9 was 5 ml for a 25-ml sample solution (Table 2). Higher volumes were not used to avoid contamination from the buffer solution.

### 3.2. Analytical performance

The FI on-line solid phase extraction/preconcentration method developed allowed the determination of Pb in the concentration range of  $0.05\text{--}0.6 \mu\text{g ml}^{-1}$  by FAAS for 120-s sample loading at  $2.2 \text{ ml min}^{-1}$ . The calibration equation was  $A = 0.0045 + 0.0534[\text{Pb}, \mu\text{g ml}^{-1}]$  ( $r = 0.9973$ ). Without preconcentration, for  $1.0\text{--}2.0 \mu\text{g ml}^{-1}$  Pb, the calibration equation was  $A = 0.0015 + 0.0021[\text{Pb}, \mu\text{g ml}^{-1}]$  ( $r = 0.9968$ ). The experimental enhancement factor, calculated from the ratio of the slopes of the calibration equations, was 25.4. The theoretical preconcentration factor, calculated as the ratio of the sample volume (4.4 ml) to the eluent volume (0.176 ml), was 25.0. The

experimental and theoretical preconcentration factors obtained for 60-, 90- and 120-s sample loading are summarized in Table 3. The agreement between the enhancement factors and the preconcentration factors is probably fortuitous as the transient signal for the FI procedure depends on the mass flux entering the flame as a function of time, which in turn is related to the kinetics of dissolution, the dispersion in the flow lines and the kinetics of the nebulizer and spray chamber response. In addition, the FI signal is generated from an ethanol solution whereas that for the conventional introduction is generated from an aqueous solution for which the nebulization efficiency is most likely different. It could be argued that, to a first approximation (equal nebulization efficiencies for water and ethanol, and rapid spectrometer response), the agreement demonstrates that for a  $176\text{-}\mu\text{l}$  elution volume the response is pseudo-steady state with the eluted lead distributed uniformly throughout the ethanol slug. Although the column lifetime was not studied in detail, no significant changes were observed in the retention properties during the course of the study (preconcentration of lead at different concentrations at least 800 times). The difference in daily absorbance values for a  $0.4\text{-}\mu\text{g ml}^{-1}$  Pb standard was not greater than 5%. The column was used as long as the same peak height absorbance was obtained (up to 20 days).

The precision expressed as the R.S.D. for nine replicate measurements of a  $0.4\text{-}\mu\text{g ml}^{-1}$  Pb solution was 2.5% for a 60-s loading time. The signals for 60-, 70-, 90-, 120-, and 130-s loading times were directly proportional to the mass of lead

Table 3

Experimental and theoretical preconcentration factors for different sample loading times

| Loading time (s) | Factor                   |                               |
|------------------|--------------------------|-------------------------------|
|                  | Enhancement <sup>a</sup> | Preconcentration <sup>b</sup> |
| 60               | 12.9                     | 12.5                          |
| 90               | 19.4                     | 18.8                          |
| 120              | 25.4                     | 25.0                          |

<sup>a</sup> Calculated as the ratio of the calibration slopes.

<sup>b</sup> Calculated as the ratio of the volumes.

introduced to the column. The limit of detection, based on the 120-s preconcentration of the ammonium acetate buffer blank, was  $2.5 \mu\text{g l}^{-1}$  (calculated as the concentration giving a net signal equal to three times the standard deviation of 10 replicate measurements of the blank signal).

### 3.3. Results for soil and water samples

The concentration found was  $1147 \pm 46 \mu\text{g g}^{-1}$  for six separate determinations of the lead in NIST Montana Soil, SRM 2711. The certified concentration is  $1162 \pm 32 \mu\text{g g}^{-1}$ . The  $\pm$  terms are the 95% confidence limits. Thus as the confidence interval for one value includes the mean of the other a *t*-test would indicate no significant difference between the values. The percent R.S.D. was 3.8% ( $n = 6$ ). This result indicated that the developed method was not affected by the potential interferences from the major matrix elements, including Al (6.53%), Ca (2.88%), Fe (2.89%), Mg (1.05%), K (2.45%), and Na (1.14%).

The procedure was further validated by the determination of Pb in tap water and artificial sea water samples. The artificial sea water contained 400–11000  $\mu\text{g ml}^{-1}$  Na, Ca and Mg as their chlorides or sulfates. The results are given in Table 4. Quantitative recoveries (94–104%) of various lead spikes were obtained, showing that the presence of high concentrations of alkaline and alkaline earth metals had no significant effect on the retention performance of Chromosorb 102 for the lead-DDC complex.

Table 4  
Analysis of artificial sea water and tap water samples spiked with Pb

| Sample               | Added<br>( $\mu\text{g ml}^{-1}$ ) | Found<br>( $\mu\text{g ml}^{-1}$ ) | Recovery<br>(%) |
|----------------------|------------------------------------|------------------------------------|-----------------|
| Artificial sea water | 0                                  | < D.L.                             | –               |
|                      | 0.100                              | 0.098                              | 98.4            |
|                      | 0.200                              | 0.191                              | 95.6            |
|                      | 0.400                              | 0.409                              | 102             |
| Tap water            | 0                                  | < D.L.                             | –               |
|                      | 0.100                              | 0.104                              | 103             |
|                      | 0.200                              | 0.196                              | 98.4            |
|                      | 0.300                              | 0.283                              | 94.3            |
|                      | 0.400                              | 0.377                              | 94.3            |

## 4. Conclusion

The studies indicate that Chromosorb is a robust and stable hydrophobic material capable of retaining lead-DDC from aqueous solution. The presence of high concentrations of Al, Ca, Fe, K, Mg and Na can be tolerated. Thus, the material has potential as a general-purpose, solid-phase extractant as it is likely that other metal DDC complexes (or other bulky, neutral, non-polar derivatives) will also be retained. As it is widely used for GC, the continued commercial availability is assured (unlike the situation for immobilized 8-hydroxyquinoline). Although the mode of retention is most likely sorbent extraction as DDC is present in excess, Chromosorb does retain metals from slightly alkaline solution in the absence of DDC and so at least one other mechanism of retention is possible. Under the conditions studied, this mechanism appears to be less efficient than the sorbent extraction; however, work in progress [23] has shown that if the retained metal is eluted with acid, enhancements in detection limits of up to two orders of magnitude may be obtained with loading up to flow rates of  $12 \text{ ml min}^{-1}$ . The material also has possibilities as a support for liquid ion-exchangers [24,25].

## Acknowledgements

The authors gratefully acknowledge The Scientific and Technical Research Council of Turkey for financial support for Dr Latif Elçi during the course of the study. This paper is funded in part by a grant from the National Oceanic and Atmospheric Administration (NOAA). The views expressed herein are those of the authors and do not necessarily reflect the views of NOAA or any of its sub-agencies.

## References

- [1] Z. Fang, Flow Injection Atomic Absorption Spectrometry, Wiley, New York, 1995.



- [2] J.F. Tyson, Atomic spectrometric detectors for flow injection analysis, *Anal. Chim. Acta* 234 (1990) 3–12.
- [3] Z. Fang, M. Sperling, B. Welz, Flame atomic absorption spectrometric determination of lead in biological samples using a flow injection system with on-line preconcentration by coprecipitation without filtration, *J. Anal. At. Spectrom.* 6 (1991) 301–306.
- [4] D. Rodriguez, P. Fernandez, C. Perez-Conde, A. Gutierrez, C. Camara, Determination of lead in natural waters using flow injection with on-line preconcentration and flame AAS detection, *Fresenius J. Anal. Chem.* 349 (1994) 442–446.
- [5] R.L. Ma, V. Van Mol, F. Adams, Determination of cadmium, copper and lead in environmental samples: an evaluation of flow-injection on-line sorbent extraction for flame atomic absorption spectrometry, *Anal. Chim. Acta* 285 (1994) 33–43.
- [6] F.M. Fernandez, J.D. Stripeikis, M.B. Tudino, O.T. Troccoli, Fully automatic on-line separation preconcentration system for electrothermal atomic absorption spectrometry: determination of cadmium and lead in sea-water, *Analyst* 122 (1997) 679–684.
- [7] E. Bulska, M. Walcerz, W. Jedral, A. Hulanicki, On-line preconcentration of lead and cadmium for flame atomic absorption spectrometry using a flow-through electrochemical microcell, *Anal. Chim. Acta* 357 (1997) 133–140.
- [8] H. Lancaster, G.D. Marshall, E.L. Gazola, J. Ruzicka, G.D. Christian, Trace metal atomic absorption spectrometric analysis utilizing sorbent extraction on polymeric-based supports and renewable reagents, *Analyst* 119 (1994) 1459–1465.
- [9] J. Ruzicka, A. Arndal, Sorbent extraction in flow injection analysis and its application to enhancement of atomic spectrometry, *Anal. Chim. Acta* 216 (1989) 243–255.
- [10] Z. Fang, M. Sperling, B. Welz, Flow injection on-line sorbent extraction preconcentration for graphite furnace atomic absorption spectrometry, *J. Anal. At. Spectrom.* 5 (1990) 639–646.
- [11] M. Sperling, X. Yin, B. Welz, Flow injection on-line separation and preconcentration for electrothermal atomic absorption spectrometry. Part 1: determination of ultratrace amounts of cadmium, copper, lead and nickel in water samples, *J. Anal. At. Spectrom.* 6 (1991) 295–300.
- [12] R. Lima, K.C. Leandro, R.E. Santelli, Lead preconcentration onto C-18 minicolumn in continuous flow and its determination in biological and vegetable samples by flame atomic absorption spectrometry, *Talanta* 43 (1996) 977–983.
- [13] R.E. Santelli, M. Gallego, M. Valcarcel, Preconcentration and atomic absorption determination of copper traces in waters by on-line absorption–elution on an activated carbon minicolumn, *Talanta* 41 (1994) 817–823.
- [14] Y.A. Zhang, P. Riby, A.G. Cox, C.W. McLeod, A.R. Date, Y.Y. Cheung, On-line preconcentration and determination of lead in potable water by flow injection atomic absorption spectrometry, *Analyst* 113 (1988) 125–128.
- [15] A.M. Naghmush, K. Pyrzynska, M. Trojanowicz, Flame atomic absorption spectrometric determination of lead in water with flow-injection preconcentration and speciation using functionalized cellulose sorbent, *Talanta* 42 (1995) 851–860.
- [16] S. Xu, L. Sun, Z. Fang, Determination of gold in ore by flame atomic absorption spectrometry with flow injection on-line sorbent extraction preconcentration, *Anal. Chim. Acta* 245 (1991) 7–11.
- [17] A. Dravnieks, B.K. Krotoszynski, J. Whitfield, A. O'Donnell, T. Burgwald, High-speed collection of organic vapors from the atmosphere, *Environ. Sci. Technol.* 5 (1971) 1220–1222.
- [18] T.C. Thomas, J.N. Seiber, Chromosorb 102, an efficient medium for trapping pesticides from air, *Bull. Environ. Contam. Toxicol.* 12 (1974) 17–25.
- [19] L.D. Butler, M.F. Burke, Chromatographic characterization of porous polymers for use as adsorbents in sampling columns, *J. Chromatogr. Sci.* 14 (1976) 117–122.
- [20] Johns-Manville Chromosorb® Porous Polymer Supports Catalogue.
- [21] R.A. Reimer, A. Miyazaki, Determination of lead in sea water by inductively coupled plasma atomic emission spectrometry combined with chelating resin preconcentration and hydride generation, *J. Anal. At. Spectrom.* 7 (1992) 1239–1247.
- [22] Z. Arslan, N. Ertas, J.F. Tyson, P.C. Uden, E.R. Denoyer, Determination of trace elements in marine plankton by inductively coupled plasma mass spectrometry, *Fresenius J. Anal. Chem.* (in press).
- [23] Z. Arslan, L. Elci, J.F. Tyson, Determination of trace elements in sea water by inductively coupled plasma mass spectrometry (ICP-MS) with on-line matrix elimination and preconcentration with Chromosorb 102, *J. Anal. At. Spectrom.* (submitted).
- [24] A. Ramanujam, P.V. Achuthan, P.S. Dhami, V. Gopalakrishnan, R. Kannan, J.N. Mathur, Extraction chromatographic separation of promethium from high active waste solutions of purex origin, *Solvent Extraction Exchange* 13 (1995) 301–302.
- [25] R. Singh, R. Khawaja, B. Gupta, S.N. Tandon, Extraction chromatographic studies of mercury(II) and some other metal ions on Chromosorb 102 loaded with triisobutylphosphine sulfide. Its application to industrial effluent, *Chem. Anal.* 44 (1999) 23–34.